

Inductance, Capacitance, Resistance, Diode

LCR METER

Model : LCR-9083



TABLE OF CONTENTS

1. FEATURES	1
2. SPECIFICATIONS	1
2-1 General Specifications	1
2-2 Electrical specifications	2
A. Inductance.....	2
B. Capacitance range	2
C. Resistance range	3
D. Diode	3
3. FRONT PANEL DESCRIPTION	4
3-1 Display	4
3-2 Power On/Off switch.....	4
3-3 Function switch.....	4
3-4 LC/R select switch.....	4
3-5 Clip input terminals	4
3-6 Direct input terminals	4
3-7 Battery Compartment/Cover.....	4
4. INDUCTANCE (L) MEASURING PROCEDURES.....	5
5. CAPACITANCE (C) MEASURING PROCEDURES.....	6
6. RESITANCE (R) MEASURING PROCEDURES.....	8
7. DIODE MEASURING PROCEDURE	9
8. MAINTENANCE	11
9. BATTERY REPLACEMENT	11

1. FEATURES

- * Digital display & battery operated, Inductance, Capacitance Resistance and Diode measurement.
- * LSI-circuit provides high reliability and durability.
- * LCD display for clear readout even in bright ambient light conditions.
- * Input overload protection .
- * Rotary switch function selector .
- * Low battery indicator.

2. SPECIFICATIONS

2-1 General Specifications

Display	18 mm (0.7") LCD, Max. reading 1999.
Measurement	Inductance : 2 mH to 2 H, 5 ranges. Capacitance : 2 nF to 200 uF, 6 ranges. Resistance : 200 ohm to 20 M Ohm, 6 ranges. Diode test
Over-input indicator	" 1 " mark indication.
Sampling Time	Approx. 0.4 second.
Operating Temperature & Humidity	0 °C to 50 °C (32 °F to 122 °F). Less than 80% RH.
Power Supply	006 P DC 9V battery, heavy duty battery.
Dimensions	185 x 87 x 39 mm(7.3 x 3.4 x 1.5 inch)
Weight	280 g/0.62 LB.
Power Consumption	R measurement : Approx. 9 mA max. L & C measurement : Approx. 13 mA max.
Accessories Included	Instruction Manual 1 PC Test alligator clips 1 pair

2-2 Electrical specifications (23 5 C)

A. Inductance

Range	In-range Display	Resolution	Accuracy	Inductor Resistance Limitation
* 2 mH	0.02 mH-2 mH	1 uH	3 % + 3 d)	< 2 ohm
20 mH	2 mH - 20 mH	10 uH		< 100 ohm
200 mH	20 mH-200 mH	100 uH		
2 H	0.2 H - 2 H	1 mH	5 % + 5 d)	< 500 ohm
20 H	2 H - 20 H	10 mH		

@ uH = micro Henry (10⁻⁶H), mH = mili Henry (10⁻³H).

@ Test frequency approx. 200 Hz.

* Zero stray inductance of 2 mH range (short circuit) :0 uH.

* The exact measuring value for the 2 mH range, should read the meter's reading value, then deduct the Zero stray inductance value (short circuit value). For example : The meter's reading is 7 uH, the short value is -15 uH, the exact measuring value is 7 uH - (-15 uH) = 22 uH.

B. Capacitance

Range	In-range Display	Resolution	Test Frequency	Accuracy
* 2 nF	10 pF-2 nF	1 pF	200 Hz	(3 % + 3 d)
20 nF	200 pF-20 nF	10 pF	200 Hz	
200 nF	2 nF - 200 nF	100 pF	200 Hz	
2 uF	.02 uF - 2 uF	1 nF	200 Hz	
20 uF	0.2 uF - 20 uF	10 nF	200 Hz	
200 uF	2 uF - 200 uF	100 nF	30 Hz	

@ pF= pico Farad (10⁻¹²F) nF= nano Farad (10⁻⁹F)

uF= micro Farad (10⁻⁶F)

* Zero stray capacitance of 2 nF range (open circuit, 30 pF

* The exact measuring value for the 2 nF range, should read the meter's reading value, then deduct the Zero stray capacitance value (open circuit value). For example : The meter's reading is 32 pF, the open circuit value is 12 pF, the exact measuring value is 32 pF - 12 pF = 20 pF.

C. Resistance

<i>Range</i>	<i>Resolution</i>	<i>Open Circuit Voltage</i>	<i>Accuracy</i>
200 ohm	0.1 ohm	Approx. DC 3 V	(2 % + 3 d)
2 k	1 ohm		
20 k	10 ohm		
200 k	100 ohm		
2000 k	1 k		
20 M	10 k	Approx. DC 1.5 V	

Remark :

a. *Though the internal test frequency is approx. 250 Hz.*

However the accuracy adjustment are executed as :

- * For the capacitance (2 uF, 200 nF, 20 nF, 2 nF) range, the accuracy adjustment is compared with the " Standard capacitor that tested under the 1 KHz frequency ".
- * For the capacitance (20 uF, 200 uF) range, the accuracy adjustment is compared with the " Standard capacitor that tested on the 100 Hz frequency ".
- * For the inductance (2 mH, 20 mH, 200 mH, 2 H) range, the accuracy adjustment is compared the " Standard inductor that tested on the 1 KHz ".
- * For the inductance (20 H) range, the calibration is compared the " Standard inductor that tested on the 100 Hz ".

b. *The above spec. accuracy are tested under the environment RF Field Strength less than 3 V/M & frequency less than the 30 MHz only.*

D. Diode

- * Short/non conductance, good/defect test
- * Approx. diode forward voltage (VF) measurement.
- * Open circuit voltage is DC 3 V.

3. FRONT PANEL DESCRIPTION

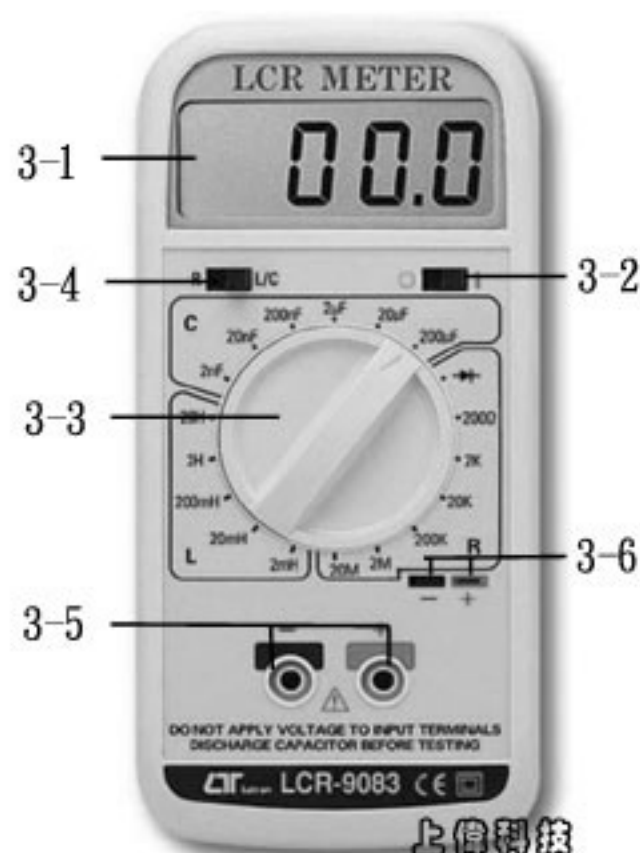


Fig. 1

- | | |
|---------------------------|-----------------------------------|
| 3-1 Display | 3-5 Clip input terminals |
| 3-2 Power On/Off switch | 3-6 Direct input terminals |
| 3-3 Function switch | 3-7 Battery Compartment/
cover |
| 3-4 LC/R select
switch | |

4. INDUCTANCE (L) MEASURING PROCEDURES

1) Slide the " Power On/Off switch " (3-2, Fig. 1) to the " 1 " position.

" 1 " = On " 0 " = Off

2) Slide the " L/C,R switch " (3-4, Fig. 1) to the " L/C " position.

3) Rotate the function switch for the maximum expected inductance range.

4) Plug the " Test alligator clips " to the " Measuring input " (3-5, Fig.1), then connect the inductor to the alligator clips.

5) Read the display. The value indicated corresponds to the range selected. If the DISPLAY shows "1", it indicates an Out-of-Range measurement. In order to improve the resolution, Select the next higher range.

NOTE:

- 1) * *If the inductance value is unmarked start with the Lower range (2 mH) and keep increasing until a suitable reading is obtained.*
- 2) * *For the 200 mH range are designed for measuring from 20 mH to 200 mH only. It is normal, if get the no convineant reading value when measue inductance less than 20 mH of 200 mH range.*
 - * *For the 2H range are designed for measuring from 0.2 H to 2H only. It is normal, if get the no convineant reading value when measue inductance less than 0.2 H of 2 H range.*
 - * *For the 20H range are designed for measuring from 2 H to 20H only. It is normal, if get the no convineant reading value when measue inductance less than 2 H of 20 H range.*

- 3) Consideration for internal circuit's stray inductance of 2 mH range, if intend to make the precision measurement, should short the input terminal first, record the display Then final true measurement value will be the " reading value " deduct above " internal circuit stray inductance " *For example : If the stray inductance is -15 uH, then the real real value is the reading value plus 15 uH (deduct -15 uH).*
- 4) Measurement of very low inductance should be performed using extremely short leads in order to avoid introducing any stray capacitance.
- 5) This instruments is not intended for determining the "Q" factor for the inductor. Misleading readings may be obtained if the measurement of the inductance of a resistor is attempted.

5. CAPACITANCE (C) MEASUREMENT PROCEDURES

- 1) Slide the " Power On/Off switch " (3-2, Fig. 1) to the " 1 " position.

" 1 " = On " 0 " = Off

- 2) Slide the " L/C,R switch " (3-4, Fig. 1) to the " L/C " position.
- 3) Rotate the function switch for the maximum expected capacitance range.
- 4) Plug the " Test alligator clips " to the " Measuring input " (3-5, Fig.1), then connect the inductor to the alligator clips.

- * ***Observe polarity when connecting polarized capacitors.***
- * ***Fully discharge any charged capacitors.***

5) Read the display. The value indicated corresponds to the range selected. If the DISPLAY shows "1", it indicates an Out-of-Range measurement. In order to improve the resolution, Select the next higher range.

NOTE:

- 1) * ***If the capacitance value is unmarked start with the Lower range (2 nF) and keep increasing until a suitable reading is obtained.***
- 2) * *For the 200 nF range are designed for measuring from 2 nF to 200 nF only.*
 - * *For the 2 uF range are designed for measuring from 0.02 uF to 2 uF only.*
 - * *For the 20 uF range are designed for measuring from 0.2 uF to 20 uF only.*
 - * *For the 200 uF range are designed for measuring from 2 uF to 200 uF only.*

It is normal, if get the no convineant reading value when measue capacitacitance :

- < 2 nF of 200 nF range.*
- < 0.02 uF of 2 uF range.*
- < 0.2 uF of 20 uF range.*
- < 2 uF of 200 uF range.*

3) Consideration for internal circuit's stray capacitance of 2 nF range, if intend to make the precision measurement, should open the test alligators (not connect the measuring capacitor), record the display (for example 15 uF it is the circuit's stray capacitance). Then final true measurement value will be the " reading value " deduct above " internal circuit stray capacitance "

- 4) A capacitor with low voltage leakage will read over range, or a much higher value than normal. An open circuit capacitor will read zero on all ranges (possibly a few pF on 2nF range, due to stray capacitance of the instrument).
- 5) Measurement of very low capacitance should be performed using extremely short leads in order to avoid introducing any stray capacitance.
- 6) When using the test leads, remember that the leads may introduce a measurable capacitance to the measurement. Capacitors, especially electrolytics, often have notoriously wide tolerances.

6. RESISTANCE (R) MEASUREMENT PROCEDURES

- 1) Slide the " Power On/Off switch " (3-2, Fig. 1) to the " 1 " position.
- 2) Slide the " L/C,R switch " (3-4, Fig. 1) to the " R " position.
- 3) Rotate the function switch for the maximum expected inductance range.
- 4) Plug the " Test alligator clips " to the " Measuring input " (3-5, Fig.1), then connect the inductor to the alligator clips.
- 5) Read the display. The value indicated corresponds to the range selected. If the DISPLAY shows "1", it indicates an Out-of-Range measurement. In order to improve the resolution, Select the next higher range.

NOTE:

In order to make precision measurement at lower ranges, deduct the stray resistance of measuring leads from the readings. The stray resistance can be measured by shorting the leads.

7. DIODE MEASUREMENT PROCEDURES

PROCEDURE

1) Slide the " Power On/Off switch " (3-2, Fig. 1) to the " 1 " position.

" 1 " = On " 0 " = Off

2) Slide the " L/C,R switch " (3-4, Fig. 1) to the " R " position.

3) Rotate the function switch for the " " range.

4) Connect red test lead to the " + " input terminal and black test lead to " - " input terminal.

Fig. 2

Fig. 3

- 5) A. When connected with polarity as shown in Fig. 2, a forward current flow is established and the approx. DIODE forward voltage (VF) values in volt will display on the display reading. If the diode under test is defective, ".000" or near ".000" value (short circuit) or "1" (open circuit) will be displayed.
- B. When connected as shown in Fig. 3, a reverse check on the diode is made. If the diode under test is good, "1" will be displayed. If the diode under test is defective, ".000" or other numbers will be displayed.
- C. Proper diode testing should include both steps A and B above.

8. MAINTENANCE

- (1) This LCR METER is intended for measuring the capacitance value of a capacitor, the inductance value of an inductor. It is not intended for determining the "Q" factor for above reactive components. Misleading readings may be obtained if the measurement of the inductance or capacitance of a resistor is attempted .
- (2) When measuring components within a circuit ensure the circuit is switched off and de-energized before connecting the test leads.
- (3) Instruments used in dusty environments should be stripped and cleaned periodically.
- (4) Do not leave the instrument exposed to direct heat from the sun for long periods.
- (5) Before removing the battery compartment cover, ensure that the instrument is disconnected from any circuit and the power switch is in the off position.
- (6) For all measurements, connect the BLACK test lead into " - " terminal and RED test lead into " + " terminal.

9. BATTERY REPLACEMENT

- 1) When the left corner of LCD display show " LOBAT ", it is necessary to replace the battery, However in-spec. measurement may still be made for several hours after LOW BATTERY INDICATOR appears before the instrument become inaccurate.
- 2) Open the screw of " Battery Cover " (3-7, Fig 1) by screwdriver, then move the battery.
- 3) Replace with 9V battery and reinstate the cover.